

ETHYLENE OXIDE STERILIZATION RESIDUALS

According to ISO 10993-7

Accredited Methods for quantification of residuals of:


- Ethylene Glycol - EG
- Ethylene Oxide - ETO
- Ethylene Chlorohydrin - ECH



WIDE RANGE
OF MEDICAL
DEVICES
that can be tested


ADVANCED ANALYTICAL Instrumentation

GC-FID Technology Gas Chromatograph with Flame Ionization Detector

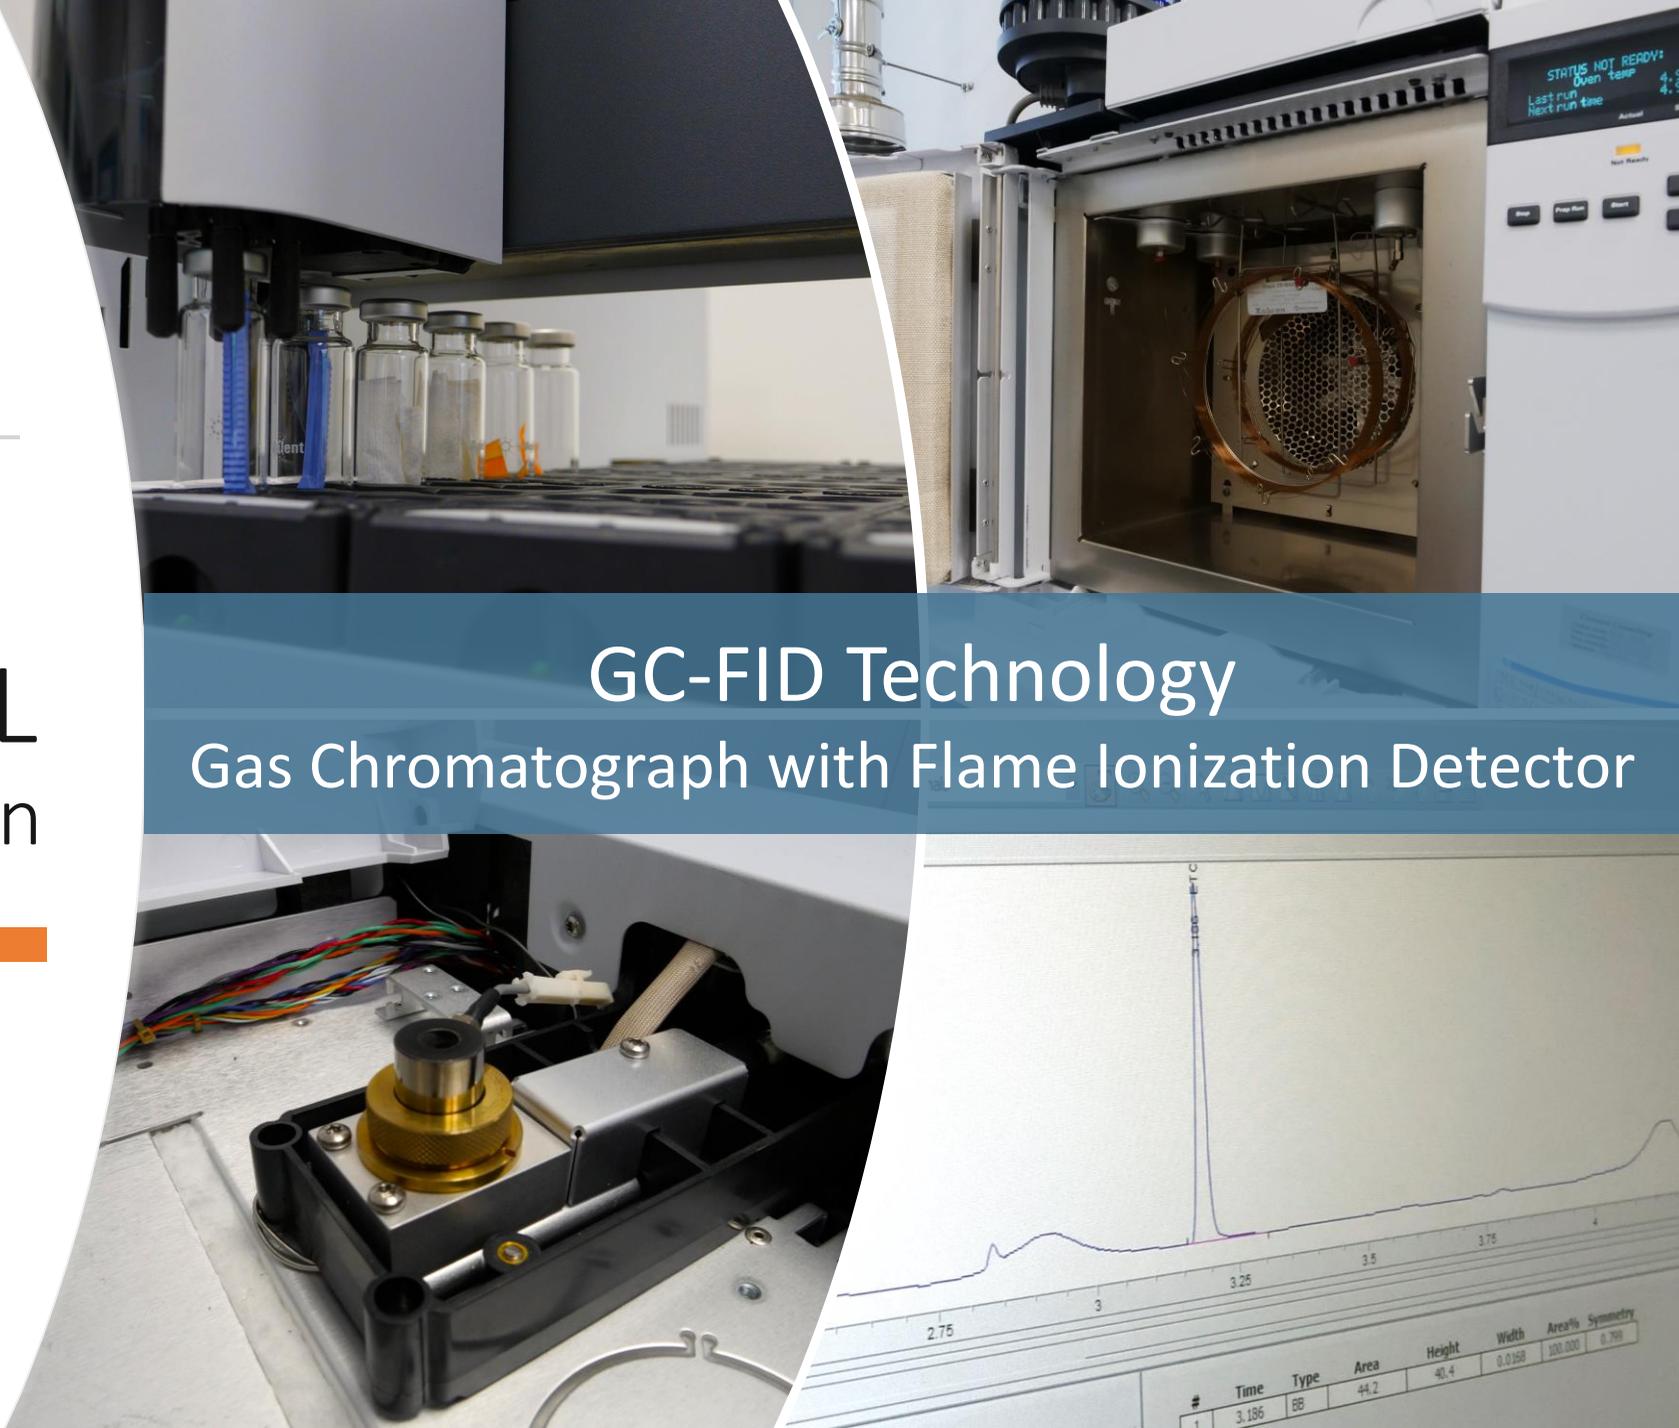

Simulated-Use Extraction

Exhaustive Extraction

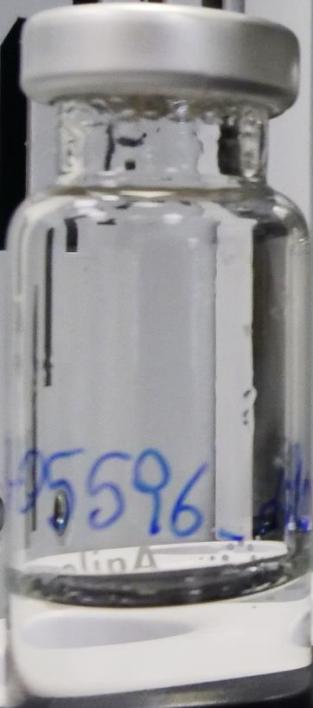

PRODUCT
EXTRACTION
METHODS

CONSULTANCY SERVICES

- Gap Analysis
- Interpretation of Results



Coronati Consulting

CONTACT US! FOR MORE INFO



Via Gavioli 3 - Mirandola (MO)
41037 ITALY



s.coronati@coronaticonsulting.it



(+39) 0535 - 611533



<https://www.coronaticonsulting.it/>



Coronati Consulting Srl